

A GUIDE FOR THE HEARING AID USERS



DEPARTMENT OF AUDIOLOGY

ALL INDIA INSTITUTE OF SPEECH AND HEARING

MANASAGANGOTRI, MYSORE - 570 006

GRAMS : "SPEECHHEARING "

PHONE : 30449 20715

INTRODUCTION

It is in YOUR hands!!

Every disability can be prevented from being a handicap. Management methods have been developed for every kind of disability. Through these methods, the deficiencies, sensory or motor can be compensated. For example 'Spectacles' have been the major line of management in case of visual impairment. Similarly, in case of hearing -impairment the major advancement in management has been in developing listening devices, namely, 'Hearing aids'

Of course, the management of hearing -impairment varies according to the type and degree of hearing -impairment. Management could be either medical or rehabilitative as in the case of reversible or irreversible cases of hearing impairment, respectively.

Just as in case of visual impairment where the selection of appropriate spectacles involves a systematic procedure, so is the case in the selection of a hearing aid. In other words, selection of a hearing aid depends upon several factors including the degree of hearing loss.

Hearing aid selection is a complex process. It cannot be selected considering just the cosmetic value or the pricetag. It is meant for a purpose! Hence, it becomes necessary that all the necessary aspects such as the degree of hearing loss, nature of hearing loss and its typical characteristics in each individual be strictly considered while rehabilitating the hearing -impaired individual.

Hence, for efficient use of hearing aid, it becomes important, that both the clinician and the beneficiary be well informed regarding the various aspects of hearing aids and its functions. This in turn will help in the maintainance and purposive use of a hearing aid, the goal being successful rehabilitation of the hearing-impaired.

Among other aspects, information on the electroacoustic characteristics of hearing aid is important for the user to have, for several reasons. A hearing aid user must know that he has a hearing aid appropriate for his needs.

Electroacoustic characteristics refer to the input-output performance of hearing aids i.e. comparing the parameters of the original sound which is presented to the hearing aid and parameters of the same sound which is recorded from the hearing aid.

A knowledge about the electroacoustic characteristics helps-

1. In knowing the performance expected of a hearing aid prior to use.
2. In differentiating among different classes of hearing aids viz., mild, moderate and strong.
3. In knowing about the performance during use and if the characteristics have changed subsequent to use.
4. In knowing the performance of a hearing aid after repair and noting changes, if any.
5. In procuring the appropriate hearing aid, appropriate to meet as prescribed by the audiologist.

It is not just the name or brand of the hearing aid according to which a hearing aid is prescribed, but a hearing aid with certain performance characteristics is important as the user is concerned. so, to know whether the hearing aid is functioning well or not, it is better to find out and have information about the electroacoustic characteristics of the hearing aid in question.

And, for efficient use of a hearing aid, it is better to know about different parts of the hearing aid and their functions.

HEARING AID: AN AID FOR THE HEARING-IMPAIRED

A hearing aid is an instrument that presents sounds more effectively to the listener's ears. It collects sounds from the environment, amplifies them and feeds to the listener's ears. It will help to hear speech or other environmental sounds, by making them louder to

the extent at which user can comfortably hear them. So, it is recommended for the use of people with hearing loss.

Thus, the function of a hearing aid is to increase the loudness of the sounds, so that they become audible by the user. A hearing aid does not improve the hearing capacity of the user, it just makes the user able to hear sounds. A hearing aid cannot be a substitute for a normally functioning ear.

Those types of hearing impairments which cannot be helped by any medication or surgery can be helped by means of hearing aid.

The day-to-day communication of a deaf person is affected without a hearing aid, as he loses contact with the environment.

Hearing aid is useful in both unilateral and bilateral hearing loss cases. Unilateral meaning hearing impairment in one ear bilateral meaning hearing impairment in both ears.

Hearing aid users must know important parts and manner of hearing aid operation, for effective usage of their aid for longer periods of time.

Hearing aid can be used for a child who is deaf since birth. It enables such children to learn to hear speech and other environmental sounds around them. It can also be used for those people who have acquired post-lingual hearing loss i.e., the cases, in which hearing loss occurs after they have learnt to talk. Hearing aid brings them back to the hearing world.


So, a hearing aid improves the loudness of speech and other environmental sounds.

There are two major types of hearing aids-body level hearing aid, and ear-level hearing aid (Behind-the-Ear).

-Body level hearing aids are worn on the body, either in shirt pocket or neck harness or clipped to the clothing. A wire (cord) runs from the aid to the receiver at the ear. They are most often rectangular in shape.

-Ear level hearing aids rest behind the ear with a plastic tube, instead of a wire (cord).


How does a body worn hearing aid look?

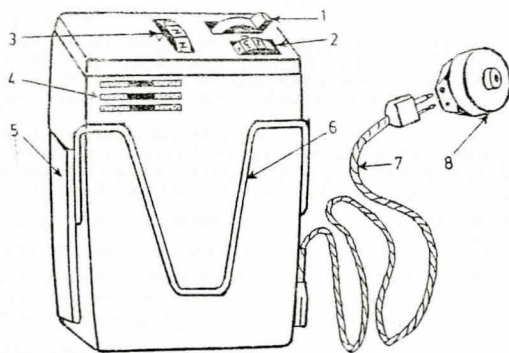

- 1. On-off switch
- 2. Volume Control
- 3. Tone control
- 4. Microphone

- 5. Battery Compartment
- 6. Clip
- 7. Cord
- 8. Receiver

How does a behind the ear hearing aid look?



1. On-off switch
2. Volume control
3. Tone control
4. Microphone
5. Battery compartment
6. Hook
7. Plastic tube

A hearing aid has many components. They are -

- Microphone
- Receiver
- Amplifier
- Power supply (Battery)


Microphone:- It picks up sounds from the environment, changes it into the electrical signal and passes it to the next part i.e., amplifier.

Amplifier:- It amplifies i.e., increases loudness of the sound with the help of power supply from the battery.

Receiver:- As the name indicates, it receives the amplified electrical signal from the amplifier, converts it into sound signal and sends to the listener's ears.

Power supply (Battery):- As in Transistor radios and Taperecorders, battery helps in functioning of the hearing aid. Amplifier needs power supply to increase the level of the sounds reaching the ear.

How sounds travel through the hearing aid to the user's ear?

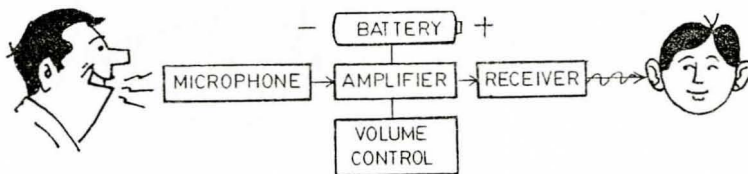

The other parts of a hearing aid are - earmold, cord, volume control, on-off switch. Accessories of a hearing aid are - tone control, telecoil.

COMPONENT DETAILS OF A HEARING AID

Earmold: An Earmold is a plastic insert that couples the receiver of the hearing aid to the listener's ear.

Microphone: Microphone is an important and delicate part of the hearing aid.

It is a device that converts acoustic (sound) energy into electrical energy.

Microphone picks up the sounds from the environment, which are then converted into electrical energy. This electrical energy is then passed further, for the process of amplification.

Location of the microphone in the hearing aid is important because the sounds closest to the microphone are picked up most readily.

Types of microphones:

Directional-These microphones pick up sounds only from one side, especially the front side of the hearing aid. They are 15-20 dB more sensitive to sounds originating from its front than the sounds originating from back. These microphones are useful, when speech signals are mixed with background noise. So, by using such microphones, a person can concentrate on the speech signals, he wants to hear, especially in noisy situations.


Omni or non-directional microphones-These microphones pick up sounds from all directions. But, the problem with such microphones is that, it picks up unwanted signals also, such as background noise. Hence, the speech signal reaching listener's ears becomes unclear.

Basically, the microphones used in a hearing aid are -


1. Magnetic
2. Ceramic or piezoelectric
3. Electret

These types are depending on the materials used inside the microphones and principles of their operation. A particular microphone is selected according to the type of hearing aid and requirements of the hearing aid. An ideal microphone should have a flat frequency response over a wide range of frequencies.

1. Magnetic:- They have a rather ideal frequency response over the range of frequencies most important for speech i.e., mid frequencies (frequencies around 1000 Hz). Very high and low frequencies are not amplified. Since the frequency response of this type of microphone is not flat over the required frequency range they are not very popular as compared to electret microphone.



2. Ceramic or Piezoelectric:- They respond equally to sounds over a wide frequency spectrum i.e., upto 20,000 Hz. They also permit amplification of extremely low frequency sounds reaching a hearing aid. But they are sensitive to shocks and drops.

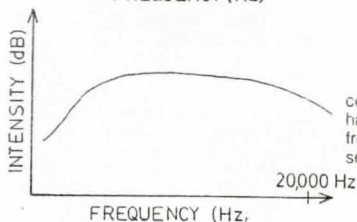

3. Electret Microphones:- They are the most commonly used microphones in hearing aids. They have a flat frequency response across a wide frequency range i.e., upto 20,000 Hz. They are less sensitive to shock than ceramic microphones.

Out of three types of microphones i.e., Magnetic, Ceramic and Electret, Electret microphones are used more commonly in hearing aids.

Amplifier:

Amplifier is the most important part of the hearing aid. It takes the weak electrical signal from the microphone and increases its power by taking extra energy from the battery attached to the hearing aid.

It consists of many small components which work together in amplification of sounds. The amount of amplification depends on the requirements of the hearing aid. In case of strong hearing aids, the amplification of electrical energy is more, so as to enable the listener to hear speech sounds at higher levels. For example, for an individual with 80-90%

hearing loss, a strong capacity hearing aid is used. In such a hearing aid, the amplification of sound is done to a greater extent than in a low capacity hearing aid which is used in hearing loss of 30 to 40%.


Two types of amplifiers may be used in the hearing aids.

- Linear (Small signal amplifiers) - Here, as the input signal level increases, there is an equivalent (linear) increase in the output signal level.
- Feedback amplifiers - In this type of amplifiers output level remains constant irrespective of the changes in the input signal. This is achieved by negative feedback. They are also called as 'Output limiting amplifiers'. They have automatic volume control. They are used for patients who cannot tolerate very loud sounds.


RECEIVER :

A hearing aid receiver is an important and delicate part of the hearing aid system. The hearing aid receiver is a small speaker, which converts the amplified electrical signal to the sound signal and feeds this sound energy to the ear.

A speaker :



A hearing aid system :

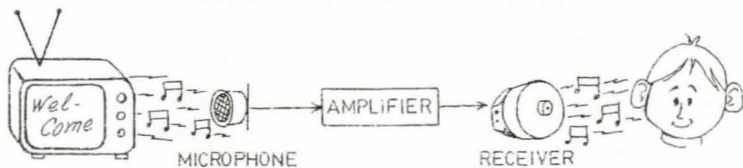


Types of receivers :

Basically, there are two types of receivers :

- 1) The air conduction receivers.
- 2) The bone conduction receivers.



1. **The air conduction type receivers**:- These are the types of receivers that are connected to the earmold and then placed in the external ear.

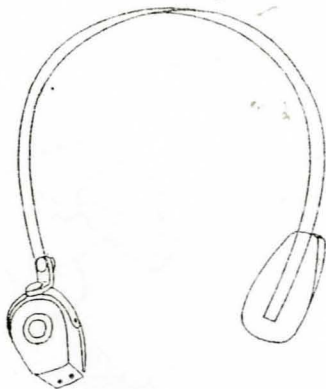

2. **The bone conduction type receivers:-** These are the types of receivers that are placed on a bone (the mastoid bone) behind the ear as in case of behind the ear.

The air conduction receivers can again be classified as -

- a) **External receivers:** These type of receivers are used in the pocket type hearing aids which are worn on the body by the user.
- b) **Internal receivers:** These type of receivers are used in behind-the-ear hearing aids.

They are also used in eye glass hearing aids that are used by those individuals with both visual as well as hearing impairment. These receivers cannot be seen outside as they are placed inside the hearing aid case.

How to achieve proper functioning of the receiver:

The maximum benefit from the hearing aid can be obtained by using the type of receiver that matches the hearing aid system, that is, there should be impedance matching between the two systems, the receiver and amplifier of the hearing aid.

What is impedance Matching?

In all electrical and electronic circuits, it is necessary that the input and output impedances should be equal or atleast in approximation. For example - The output impedance of microphone should be equal to the amplifier input and output impedance of the amplifier should be equal to the receiver impedance.

The term impedance means, reactance (resistance) to current in a circuit, i.e., it is the obstruction to the flow of sound energy/electrical energy.

In hearing aids, the impedance of the amplifier should match the impedance of the receiver for maximum transfer of energy from amplifier to receiver. If this condition is not satisfied then there would be impedance mismatch between the circuits of two devices, which results in -

- 1) Loss of signal
- 2) Distortion of signal.

For example: Impedance of the amplifier = X
Impedance of the receiver = Y

- a) Impedance matching - $X = Y \rightarrow$ maximum transfer of energy.

o) impedance mismatch :

- i) X is higher : The output would be less, so less output from the receiver.
- ii) Y is higher : Though amplifier is allowing smooth flow of energy, as impedance of receiver is high, the output will decrease.

So, in a hearing aid, for the most effective output of sound signal, there should be impedance matching between the components of a hearing aid.



WASHERS:

The washer is a small perforated disk of metal, rubber or plastic used to tighten the joints.

Plastic washers are used in hearing aid receiver to remove the gap between the receivers and earmolds, to prevent leakage of sound energy reaching the ear.

Plastic and Metal rings:

The earmolds have a hole at the base, to which the receiver is fixed. This hole is bounded by a ring which can be made of plastic or metal. Selection of the ring depends on the case's requirements.

Plastic rings are lighter, and comfortable. But they are less durable and ring fixing is cumbersome. The earmold should have larger hole for fixing plastic ring, so if the base of the mold is smaller as in the case of children, then this ring cannot be used. The Diameter of newly developed plastic ring is not big and hence can be fixed to earmolds of small children.

Also, in those people, who stay at far off distances and cannot visit the clinic very often, plastic rings cannot be used because of their shorter durability.

Metal rings last longer and fixing of these rings is not much cumbersome. So, they can be used in children and patients who stay at a distance from the place as they have longer durability.

Points to be considered in purchase of receivers :

1. Which type of receiver to buy i.e., air conduction or bone conduction receiver.
2. The user should purchase a receiver prescribed by the audiologist i.e., always a matching receiver should be purchased.
3. Washer on the receiver should be intact, to avoid leakage of sound energy.

Cell: Hearing aid requires a battery for its operation. Different types of hearing aids use different types of batteries. For example, a body level hearing aid requires a pentorch (R6) cell for its operation. Similarly, BTE requires a button cell for its operation.

Size: Hearing aid cells come in various sizes. For body worn hearing aids, cells used are similar in shape. They are the cells used in smaller flash lights and are called 'Pentorch cells', commonly they are also known as 'pencil cells'.

But for a hearing aid worn behind the ear or in the ear or spectacle type hearing aid, much smaller cells are used, which are flat and round like a button, so are known as 'Button cells'.

So, every hearing aid user must remember that he should use the appropriate type of cell for his hearing aid, to get the best from his hearing aid.

Voltage: Every hearing aid user should see that a cell provides the necessary voltage required for functioning of hearing aid. Usually, the pentorch cells and button cells (non-rechargeable) type are designed to give 1.5 volts at 450 mah and 1.35 V 80 mah respectively. When the cell voltage goes below 1.2 volts, the cell has to be replaced.

Cell life: How long a cell lasts, depends upon the power requirement of a hearing aid. In a strong hearing aid, the cell life will be less than a moderate hearing aid i.e., the

cell life depends upon the efficiency of the microphone, the amplifier and the receiver of the hearing aid and also on the volume control setting.

Process of recharging: Generally nickel-cadmium cells are rechargeable. These cells are rated for 1.2 volts instead of 1.5 volts at 450 mah. To get maximum life from these type of cells it is a good practice to recharge these cells before voltage drops below 50% rated voltage. a rechargeable battery can be charged upto 500 times.

Points to remember:

1. Maximum cell life can be achieved with daily use and daily recharging.
2. Charging requirements should be met daily regardless of hours of use, it ensures that the cell is never completely discharged. A cell should atleast be charged once in three days, if it is kept without recharging for more than three days, it gets discharged.
3. A cell should be charged at the rated current for specified number of hours.
4. Recharged cell lasts for approximately 12-18 hours depending on hearing aid type.
5. After repeated recharge, i.e., say after 500 times of recharging process, cell gives short life and so it must be replaced.

Guidelines for the effective use of a hearing aid cell:

1. Each cell is marked with + & - marks for its terminals. Similarly battery compartment is also marked with + and -marks for its terminals. When one places the cell in the battery compartment he/she should ensure that + marking of the cell corresponds to + marking on the battery compartment.
2. Before replacing the cell in a hearing aid, the hearing aid should be switched off.
3. The cell should be removed from the hearing aid, if the aid is not being continuously used, otherwise hearing aid constantly consume current from the cell. Hearing aid may also get damaged, if the cell starts leaking.
4. If the cell terminals or contact surfaces get corroded, they can be cleaned with knife or blade, gently.
5. The user should always keep a spare cell with him.

Once the hearing aid use has been stabilized, he should keep track of the average life of the cell. It can be decided depending on for how many hours in a day he uses the hearing aid. This average serves as a figure to alert the user to the time, when the cell functioning may fail.

EARMOLD:

An important part of the hearing aid is individually molded earpiece or insert. It is made of a material called 'Acrylic'.

The earmold physically attaches the hearing aid to the delicate parts of the ears and is designed to conduct the amplified sound from the output receiver of the aid into the ear canal as efficiently as possible. It seals off the ear canal to help in eliminating the annoying squeal sound sometimes heard from a hearing aid which might interfere with speech perception and to fit the receiver efficiently in the ear.



So, the earmold is more than just a sound channel, a good earmold will maintain the important balanced envelope of sound selected for the user and provide utmost comfort to the user.

If not coupled properly, it affects sound energy reaching the ear.

Ways of making earmolds:

1. Custom earmolds:- They are made from the impression taken of the hearing aid user's ears, both right and left ear.
2. Standard earmolds:- They come in various sizes and person can choose the appropriate earmold depending on his ear size.

It is better to have custom earmolds as they are exact copy of an impression of an individual person's ear, so they fit properly. Standard earmolds may not fit properly in the ear.

Another type of ear insert is provided by the hearing aid dealer which comes in the form of a ear-tip or a small plastic tube. But they don't fit properly in the ear and may fall off. So, it is always advised to use a custom earmold with the hearing aid. Facilities for making custom earmolds are available at some of the speech and hearing centres.

How to attach receiver to the earmold?

The receiver is made with a small tube like projection at 'nub' on its face that snaps into a recess in the earmold and is held there by a ring in the earmold. The sound passes through this nub and through a hole drilled in the earpiece and is delivered well down in the ear canal of the ear.

Different earmold styles in use today are -

There are different special types of earmolds that are used with different hearing aids, as -

- 1) Receiver mold - is used with both body level and ear level hearing aids with an external receiver.
- 2) Shell mold - is used for hearing aids with internal receivers, used with very high gain ear level hearing aids.
- 3) Skeleton mold - used with moderate gain ear level hearing aids.
- 4) Canal mold - used for moderate gain ear level hearing aids and has maximum cosmetic appeal.
- 5) Canal lock mold - used with moderate gain hearing aids and allows proper fitting of the earmold inside the ear.
- 6) All-in-the ear mold - designed to couple and hold in 'all in the ear hearing aid' in the ear.

According to the requirements of the user and type of hearing aid used, earmold is prescribed. But, it is always better to have custom earmold, as it is the impression taken of the individual's ears.

Purchase of the earmold:

- 1) Appropriate type of earmold should be purchased.
- 2) In case of custom earmolds, even in standard earmolds, it should fit properly in the ear.
- 3) Receiver should fit properly into the earmold, so that the receiver does not revolve. If it does revolve, the ring of the earmold should be got fixed properly.
- 4) Earmold should not be broken, even if one part is broken, it will not fit properly into the ear and may fall off.

CORD :

The cord is a thin flexible wire that carries the amplified signals from the amplifier to the receiver, i.e., it connects the amplifier with the receiver.

As the ordinary electrical wire carries the electrical energy, the hearing aid cord also carries the electrical energy from the amplifier to the receiver. (It is a very thin, flexible and delicate part of the hearing aid.) At both ends of the cord, plug pins are attached to connect it with the hearing aid and receivers. It is a preformed wire which cannot be repaired for its re-use.

Pins of the cord :


Hearing aid cord has either two pins or three pins, like a regular plug pin. In two pin plug one pin is thick and the other one is thin. In three pin plug centre pin is longer than two side pins.

Types of cords :


- There are three types of cords as :
- 1) Single or 'S' cord.
 - 2) 'V' cord.
 - 3) 'Y' cord.

The use of the cords depends upon whether a single receiver or two receivers are used. With a single or 'S' cord, one receiver is used. With 'V' or 'Y' cord, two receivers are used. 'S' and 'V' cords are used more commonly. 'Y' cord is used rarely.


Single cord is used in cases who need hearing aid in one ear only, while V or Y cord is used in cases who need hearing aid in both the ears.

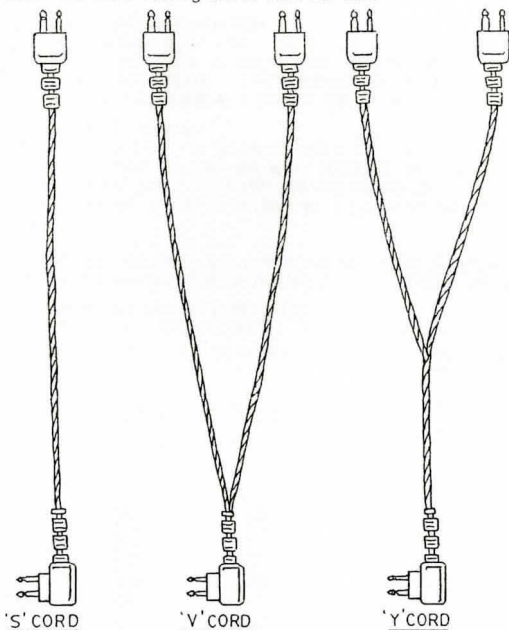

One end of the cord is connected to the body of hearing aid, called as 'angle flex' point. The other end is connected to the hearing aid receiver, called as 'adiflex' point.

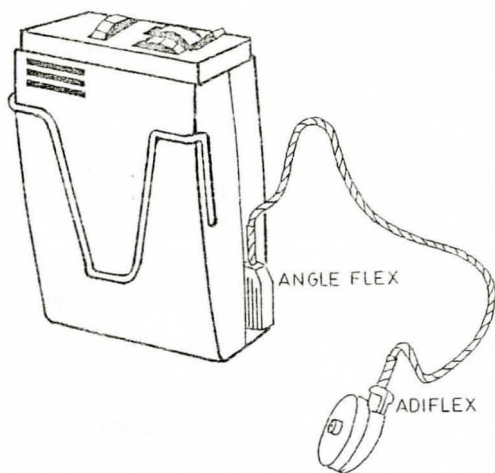

Minimum length of the hearing aid cord according to ISI should be 50 cms. Such a cord is used in the hearing aids which are pocket type i.e., worn on the body of a person.




In some types of hearing aids worn behind the ear, instead of such long cords, flexible plastic tubing are used for conduction of the sound energy.

Purchase of the hearing aid cord: Points to be noted -

- 1) Whether it is 'S', 'V', or 'Y' cord as prescribed by the audiologist.
- 2) Whether it is 2 pin or 3 pin cord.
- 3) Cord should be checked carefully to detect any breaks along its length.
- 4) Length of the cord should be 50 cms.

- 5) User should ensure the type of the cord i.e., whether he requires AF1 or AF2 which is shown in the figure.




Care of the cord:

- 1) As it is the most delicate part of the hearing aid, it should be used carefully.
- 2) In body level hearing aids, aids are placed away from the receiver as far as possible without straining the cord to avoid squealing.
- 3) The cord should not be knotted, twisted or coiled, as it causes breakage in the cord, results in intermittent contact. Cord should not be twisted or pulled.

VOLUME CONTROL:

It is similar to a volume control on a radio or a T.V. A hearing aid user uses to adjust the sound intensity he is receiving. The volume control helps to adjust the amplification, however, it does not alter the input sound to the aid. It just helps to adjust the amount of amplification of the input signal i.e., gain of the hearing aid, most useful for the hearing aid user.



Most of the hearing aids have a dial or serrated wheel that serves as a volume control. It has numbers marked on it, to indicate the level of the output of the hearing aid reaching the ears. Usually, the numbers range from 1 to 8 or 9, 1-indicating minimum gain 9 indicating maximum gain.

Care of the volume control:

1. Volume control wheel is also delicate, so it should be handled gently.
2. It should be kept on the position advised by the audiologist.
3. It should be cleaned regularly by a brush.

ON-OFF SWITCH:

Equipments like radio, T.V., tape recorders have on-off switch. In the same way, hearing aids also have on-off switch to make and break the circuit depending on the position it is placed. When the switch is on the 'ON' position, it allows the passage and amplification of the sound i.e., hearing aid functioning. When the switch is in the 'OFF' position, it breaks the circuit, thereby stopping the hearing aid functioning. Hearing aid should be switched off, if the hearing aid is not in use. Before switching on the hearing aid, volume control should be kept in the minimum position. It should be switched off, while changing spare parts of hearing aids as battery, cord, receiver or earmold.

Switch should be intact, any breakage would hamper hearing aid functioning.

ACCESSORIES OF THE HEARING AID

i) Tone Control:

Tone control is one of the important switches of the hearing aid. Tone control consists of different filter networks which transmit only a band of selected frequencies of signal from


microphone to amplifier. It controls the tonal quality of the output. Tone control switch helps to select different types of such filters such as L, N, H.

Internal Structure :

Tone control is marked H, L, N. 'H' being high frequency emphasis, 'L' being low frequency emphasis, 'N' Normal i.e., no special emphasis on the high or low frequencies.

Function :

Thus, if the user needs more of high frequency emphasis, he may be advised to turn the tone control to a position marked 'H'. For low frequency emphasis, tone control may be adjusted to 'L', otherwise to 'N'. The tone control should be set to the position prescribed by an audiologist for best performance.

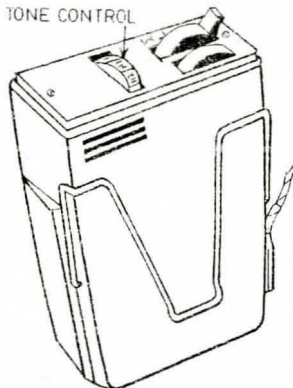

ii) Telecoil

Hearing aids with telephone pick-up coil or telecoil is an advantage because they allow the user to use the telephone without the interference from background noise.

Mode Switch :

Hearing aids with this component have either a two or three position switch that allows use of the microphone alone, i.e., 'M', the telecoil alone 'T', or both together 'MT'. If the switch is adjusted to 'T' position, the microphone i.e., 'M' is cut off. 'MT' means the user can listen to the telephone and also the background speech i.e., normal conversation can be used simultaneously.

When the switch is adjusted to 'T' position, the telephone receiver should be held against the microphone of his hearing aid and not on the ear of the user.

Thus telecoil is a very useful option for those hearing-impaired who are frequent telephone users.

Use :

Every user must learn about telecoil manipulation and switch position. Otherwise, the switch may be inadvertently moved to the telecoil position, in which case the hearing aid, in general use, will deliver no useful signals.

DECIBEL

Most of the quantities are measured in fixed units as feet, meter, kilogram, etc. For example, when we say that the distance between two points is 20 meters, we mean that the distance between the points is 20 times greater than one meter. For measuring sound intensity we use a unit, watt/cm².

But, it is convenient to measure sound intensity along the 'decibel scale'. It is most often denoted as 'dB'.

Decibel is a very important term for a hearing aid user, as the amount of hearing loss he has, is expressed in decibels. Also the gain of a hearing aid is expressed in decibels. How powerful a hearing aid is, is also measured in decibels. Thus, decibel is an important concept to become familiar with.

Decibel is not an absolute or fixed unit such as grams, meter, feet, but still, it is convenient to use. It is expressed in logarithmic scale. It refers to a logarithmic ratio between two quantities. It is a ratio between two quantities, a measured quantity and a quantity used as a reference. The quantity used as a reference is predetermined. For example, if the measured quantity is 25 and the reference point is also 25, the ratio will be $\frac{\log 1}{\log 1}$ ($25/25 = 0$).

Thus, in case of hearing aids, the dB gain is the ratio between a measured quantity i.e., the output of a hearing aid (level of sound that is coming out of the hearing aid) and the reference point i.e., the input to the hearing aid (level of the sound that is entering the hearing aid). This calculation helps one to know the amplification capabilities of a hearing aid.

ELECTRO-ACOUSTIC CHARACTERISTICS OF HEARING AID

Electroacoustic characteristics help in knowing the input-output performance of the hearing aid, and depending on these performance characteristics a particular hearing aid is prescribed. These characteristics are as follows:

Gain:

Gain is an important characteristic of a hearing aid, that the user must know about.

Gain is defined as the increase in the signal power that is produced by an amplifier usually given as the ratio of output to input voltage, expressed in decibels.

Gain is measured by determining the difference in decibel between the level of the input at the microphone and the level of the output at the receiver. For example, if input = x and the output = y, then gain is = (y-x) dB i.e., (o/p-I/p).

Gain is the term used to describe an increase in loudness of a signal as in hearing aids. Gain of the hearing aid is the amount of amplification, it provides. Thus, it gives an idea as to how much of a boost, a hearing aid can give to sounds. The unit of gain is decibel (dB). Gain of a hearing aid is expressed in numbers as 30 dB, 45 dB etc. A higher number indicating higher gain.

Depending on their gain, hearing aids can be classified into different categories, as mild, moderate and strong hearing aids. This classification has been derived on the basis of hearing impairment levels in the audiometer i.e. for selecting a hearing aid that has a gain equal to the hearing level established by the audiometric tests.

The gain of a hearing aid is adjustable with the help of volume control. As the volume control is increased, the amount of gain also increases. But once the volume control is rotated beyond 50% of the total range, the amount of distortion increases.

Determination of the amount of gain required by a hearing impaired individual is based upon 'most comfortable level' of a patient i.e. it is the level at which the patient does not have to put extra effort in listening and sounds are amplified appropriately to fulfill the user's requirements. The sounds are not too soft or not too loud.


The signal sent through a hearing aid for calculating the gain, is a series of puretones of varying frequencies, but all being at the same intensity level.

Type of gain:

Gain of a hearing aid can be measured in different ways. They are taken into consideration by a hearing aid manufacturer in the process of manufacturing the hearing aids. They are -

- 1) Peak gain
- 2) Average gain
- 3) High frequency average gain.

1) **Peak gain**:- It refers to the maximum gain of a hearing aid. It is the point on the gain curve at which the gain is maximum. It is important to know the dB level of the peak gain and also the frequency at which it occurs. Example -

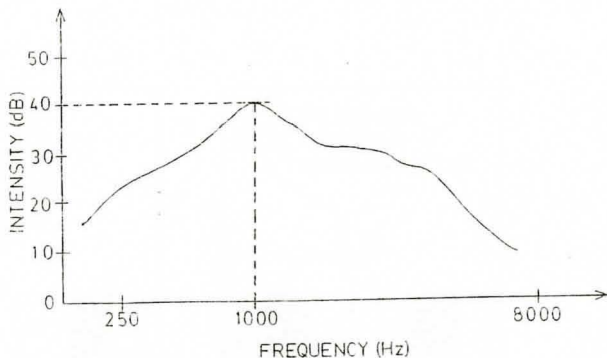


Peak gain = 40 dB at frequency of 1000 Hz.

It is important because the user's comfort setting a hearing aid will be determined, primarily by the peaks in the response. For example - If a particular patient requires a hearing aid with a peak gain of 50 dB, but the aid used has a peak gain of 40 dB. In this case the gain of the user's hearing aid will be reduced because of the peak, which might result in insufficient amplification for the patient.

The user should find out this peak gain of his hearing aid and the frequency at which it was obtained.


2) **Average gain**:- It refers to the average value of the gain at three frequencies. The average gain is measured at 500 Hz, 1000 Hz and 2000 Hz. Example -

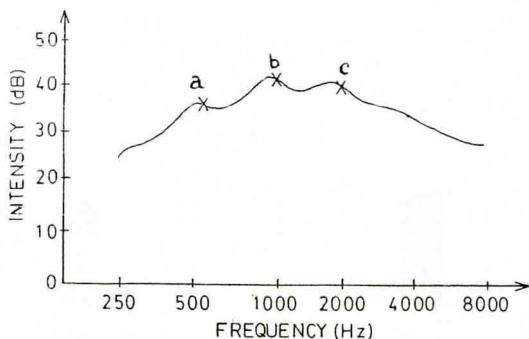

$$\text{Average gain} = \frac{a+b+c}{3}$$

3) **High frequency average gain or HF average gain**- HF average gain refers to the average value of the gain at three higher frequencies i.e. 1000Hz, 1600 Hz and 2500 Hz. Example -

$$\text{Average gain} = \frac{a+b+c}{3}$$

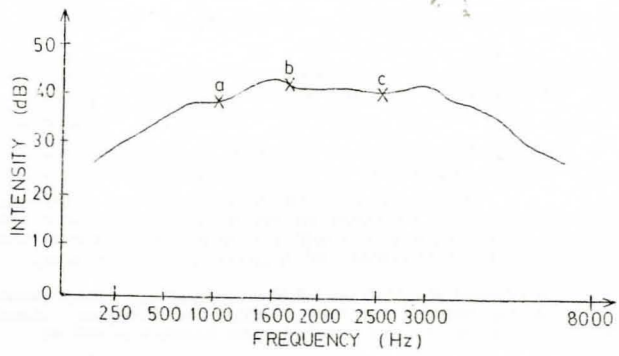

There are three more parameters that are used by a clinician in prescription of a hearing aid in collaboration with the three previous parameters: they are -

- 1) Functional gain
- 2) Insertion gain
- 3) In-situ gain



1) **Functional gain** - Functional gain is the difference between the unaided and the aided responses of the hearing aid user at the audiometric frequencies (i.e. from 250 Hz to 8000Hz).

Here, meaning the responses of the user without the hearing aid and aided are the responses of the user when he is wearing a hearing aid.

Functional gain is measured behaviourally. It is a subjective method of measurement as the responses depend upon the user.

Unaided Threshold


Aided Threshold

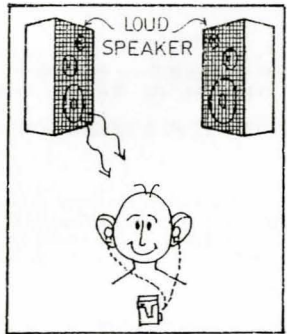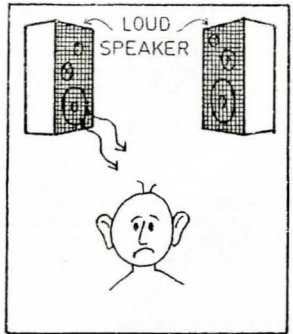


2) **Insertion gain** - It is the difference between the sound pressure level measured near the eardrum, with and without a hearing aid.

It is measured electroacoustically, i.e. it is an objective method of measurement of gain, where the user does not have to indicate the response, they are recorded with the help of an instrument.

Unaided Threshold


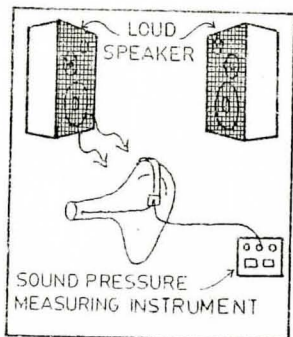


Aided Threshold

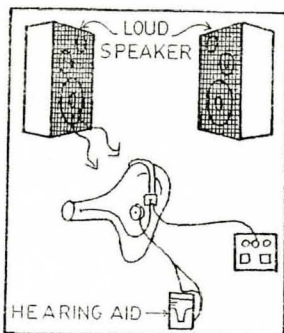

3) **In-situ gain** - It is the difference between the sound pressure levels at the eardrum of the patient using a hearing aid and a free-field sound pressure level at the position of the subject, when the subject is not present.

In-situ Gain

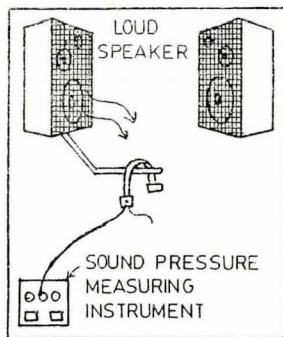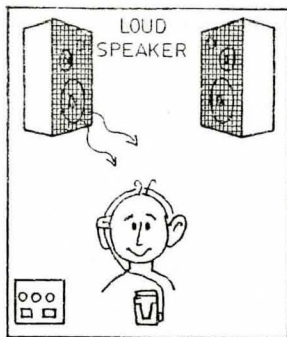

It is measured electroacoustically, i.e. it is an objective method of measurement.

Gain of a hearing aid varies across frequencies depending on the characteristics of individual hearing aid. It differs depending on the parts used in construction of a hearing aid so the gain at some frequencies may be more than others i.e. the hearing aid may boost certain frequencies to a greater extent. A hearing aid can be designed to give more gain at higher frequencies and less at lower frequencies or vice versa, depending on the user's requirements.

Automatic gain control hearing aids-

In some hearing aids, a special circuit may be added, to automatically reduce the gain when sound crosses the present limit of the hearing aid.

This is done so that the sound level reaching the hearing aid user does not cause pain to the user. Such kind of circuits are used in some special hearing aids as 'automatic gain control hearing aids', which are given to people who cannot tolerate very loud sounds i.e. even if the sound reaching the microphone of a hearing aid (input) is very loud, the output is automatically controlled to reduce the gain of the hearing aid, so that it does not cause discomfort to the user.

Based on gain, different hearing aids can be categorised as mild (31 - 52dB), moderate (41 - 62dB) and those strong (58 dB and above).

Gain characteristics are considered in terms of the client's hearing loss and the amount of amplification needed to compensate for that hearing loss i.e. a person with a mild hearing loss would not be a candidate for a hearing aid in the strong category as it would be too powerful for him. At the other extreme, a mild gain hearing aid would not be selected for the individual with a severe hearing loss, as the hearing aid would not be able to provide sufficient amplification to compensate for the loss.

Body worn hearing aids are designed to help individuals with mild, moderate and severe impairment, as they come in all these categories i.e. mild, moderate and strong gain hearing aids.

Behind the ear hearing aid are designed to help most individuals with mild moderate hearing impairment, the gain of the hearing aid being upto 65 dB.

In - the - ear hearing aids can provide the gain values upto 45 dB i.e. can be used to help the individuals with mild hearing -impairment.

Another type of hearing aid is Eyeglass hearing aids, where hearing aid circuit is mounted inside the rim of the spectacles. It can be used in those individuals who have a dual impairment i.e. visual and hearing. Gain of such hearing aids is upto 65 dB, it can be used with the persons having mild to moderate hearing - impairments.

Summary:

Thus, in manufacturing of hearing aids, 3 types of gains are involved as

- peak gain
- average gain
- high frequency average gain.

A clinician makes use of three more types of gains in addition to the above three, for prescribing a particular hearing aid. These are -

- functional gain
- insertion gain
- in - situ gain.


Hearing aids can be categorized as mild, moderate and strong gain hearing aids depending on their output characteristics.

FREQUENCY RESPONSE:

Sounds of various frequencies reach the hearing aid microphone. These sounds can be of low frequencies i.e. low pitched or high frequencies i.e. high pitched or those which fall in between these two, they are mid-frequency sounds. The hearing aid may not amplify all the sounds to the same extent, it shows preference for some frequencies by making them louder, while other sounds are not made louder to the same extent. Depending on the nature of the components of a hearing aid, some frequencies of sound signal are amplified more efficiently than others. This relation between the frequency and amplification gives the frequency response. It is a graph of acoustic output of a hearing aid against the frequency of the input signal. This graph depicts, for each frequency, the amount by which the instrument amplifies the incoming signal. In this frequency response curve, the pattern of amplification provided by the hearing aid may be varied according to its components.

As we measure the hearing sensitivity of the individual, so do we measure the sensitivity of the amplifying system at each frequency, in a frequency response curve.

To find out the frequency response of a hearing aid, sounds of different frequencies can be sent through the microphone at one end and measured at the other end, when they come out of the receiver. This graph can be shown as -

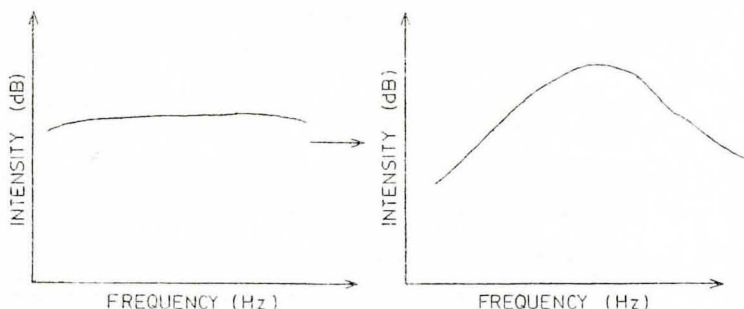

(Hertz - Hz being unit of frequency)

The standard frequency response is generally obtained at a lower gain setting i.e., volume setting than the maximum possible setting. Frequencies from 300 Hz to 5000 Hz are all sent in at the same intensity level. Frequency response characteristics of many aids do not, generally, extend beyond this range, as good comprehension or understanding of conversational speech, can be achieved within this range of 300 Hz to 5000 Hz.

Though frequencies from 300 to 5000 Hz are sent in at the same intensity level, when they are measured on coming out of the receiver, some frequencies are found to be at a higher level than the others, giving a frequency response curve.

FREQUENCY RANGE:


The frequency range of an aid refers to the useful range of the frequency response. It is expressed by two numbers, one representing the low frequency limit of amplification and other high frequency limit, both the numbers are expressed in Hertz (Hz).

Thus, from the frequency response curve, the frequency range for the hearing aid can be calculated.

With each hearing aid, the manufacturers are expected to supply the information regarding the frequency range of the hearing aid. The user must be aware that the frequency response of the hearing aid and for calculating the frequency range, standards are specified by the National Standards Institution. Also, the hearing aid user may ensure that the frequency range specified by the manufacturer is measured and calculated as per the prescribed procedure by this Institution.

SATURATED SOUND PRESSURE LEVEL OR MAXIMUM OUTPUT LEVEL (SSPL) :

It is the sound pressure level obtainable in the coupler from the receiver of a hearing aid at any frequency from 200 Hz to 8000 Hz. It is the output level that cannot be exceeded, regardless of how far the gain control or volume control is turned or how intense the input signal is i.e., even if the input is increased or gain control is turned to maximum, the output does not exceed certain level. Maximum sound pressure level at all frequencies must be less than the sound pressure level that causes discomfort or pain at that frequency. The graph of maximum sound pressure level is as follows :

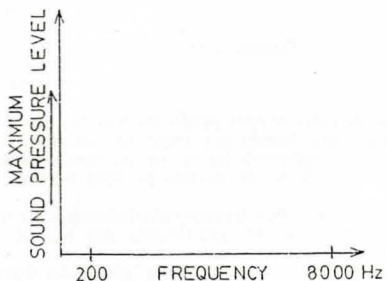

This maximum output can be used as a safety factor against sounds that might be harmful or uncomfortable.

EQUIVALENT INPUT NOISE LEVEL :

This term refers to the noise heard from the hearing aid, even when there is no sound reaching the microphone i.e., the difference between the noise when there is input and no input is the noise generated by the circuitry of the hearing aid. The moment a hearing aid is switched on this sound starts coming.

This sound should not exceed the maximum limit that is specified in the standards for a particular model of a hearing aid. These standards may be national or international.

DISTORTION :

Distortion occurs in the hearing aid, when the output signal differs from the original signal, in other words, distortion occurs when input signal is not faithfully reproduced.

As distortion increases, it becomes difficult to identify the original signal. Therefore, distortion should not exceed a particular limit, which is usually expressed in percentage. For example, if the limit is x%, then it means that the level of the distortion products should not exceed x% of the level of the original signal. Thus, the word distortion refers to any change in the original sound signal.

Types of Distortion :

The main types are : Harmonic distortion and Intermodulation distortion.

But only harmonic distortion is included in the present Bureau of Indian Standards pertaining to hearing aids as it is easily measured.

A harmonic distortion occurs when the output signal contains sounds of frequencies that are multiples of the original sound frequency. For example, if the input to a hearing aid is a 1000 Hz signal then harmonic distortion would cause a signal to be produced by the hearing aid at 2000 Hz, at 3000 Hz and so on, even though these were not part of the signal presented to the hearing aid.

Percentage of distortion for a particular frequency provides the range in which new frequencies have been generated. Here, new frequencies refer to those frequencies that were not present in the input signal.

3% of distortion at 500 Hz means 2nd harmonics (1000 Hz) and 3rd Harmonics (2000 Hz) have been generated in the circuit for the input of 500 Hz. The average percentage of distortion at these harmonics are considered as distortion at 500 Hz.

Distortion permitted at each frequency may be obtained from the 'National Standards Institute' or from your Audiologist.

Measurement of these electroacoustic characteristics need special instrumentation. Some of the speech and hearing centers and dealers of the hearing aids may have this instrument. Every hearing aid manufacturer must specify values of all these characteristics for all the hearing aids, so that the hearing aid prescription becomes an easy procedure.

GUIDELINES FOR PURCHASE OF HEARING AID

Choice of a good hearing aid is the first step in the rehabilitation of a patient with hearing loss. By means of a hearing aid, the residual hearing is made maximum use of. A hearing aid does not restore hearing to normal i.e., it is not as if, new ears have replaced the damaged ones. The amount of benefit derived from the use of a hearing aid varies from individual to individual.

The hearing aid user must know that the benefit derived from the aid is limited, so he/she should not get disappointed after the purchase of the hearing aid. To what extent, the use of a hearing aid is beneficial in an individual case may be ascertained at the time of hearing aid trial.

Hearing aid helps in detecting the presence of sound and in understanding speech. Thus, it helps in becoming aware of the danger. So, the hearing aid would serve to warn the users of approaching vehicles.

All hearing aids are not alike. Some are worn in the pockets with the receiver in the ear, some may be worn behind the ear. Some look like spectacles but also have the necessary components to make the sounds louder for the patient with hearing loss. Some hearing aids are very small which are worn inside the ear, and are not noticeable easily. Some are big enough to be noticed very easily.

Hearing aids vary in terms of their size, appearance and also in terms of how powerful they are. The type of hearing aid for a patient is determined by his/her needs, desires and financial status.

All hearing aid purchasers/users must have medical examination of their ears before purchase of a hearing aid for the well being and safety of themselves. Such an examination should also be followed periodically; say after every six months or one year.

Thus, hearing aids are normally recommended when -

- 1) Medical/surgical treatment is not indicated to revert the hearing to normal.
- 2) Surgical treatment is decided against for a number of reasons.
- 3) Surgical/medical treatment is given but improvement in hearing is not sufficient to preclude use of a hearing aid.
- 4) Surgery is possible, but the patient opts for a hearing aid.
- 5) Surgery is awaited and hearing aid is to be used in interim period.

In all such cases, selection and acquisition of hearing aid becomes essential for the individual with hearing loss.

Points to be noted:

- 1) Before purchase, the user must have a trial with different types/models of hearing aids to choose the one that gives him/her the optimum benefit. For this reason, prior to purchase of a hearing aid, the potential user must visit a speech and hearing professional, where he would have the opportunity to try out different models and seek professional guidance. Hearing aids must be purchased only on the recommendation of a qualified professional i.e., an Audiologist.
- 2) Before purchasing, the user must first ascertain that this particular model provides him the required help. Though, cosmetic value is important, it should not outweigh the consideration of amplification needs.
- 3) It is useful to know, how powerful a hearing aid is and also some other characteristics. More powerful hearing aid must not be the one always preferred. Purchase of a hearing aid, that is more powerful than the one actually required by the user must be avoided.
- 4) Different models of hearing aids can be purchased within the country. Some users may feel that if a hearing aid is imported or otherwise got from a foreign country it would serve them better. Such user must remember that - (a) It is preferable to purchase an aid after a hearing aid trial (b) Hearing aid requires periodical servicing and replacing of spares which may be more difficult to procure for the imported hearing aids. And, the spares of these hearing aids may not be available in our country.
- 5) Here, one more important point is, it is not wise to buy a hearing aid by mail, if there is any practical alternative. Direct personal contact with the dealer is most desirable, as nearness of a dealer is a great advantage for inspection and trial of a hearing aid. It is also useful for subsequent repair and replacement service.
- 6) Also, specific inquiry should be made about the availability and quality of the spares and cost of service, including the replacement of cells.

Repairs and Servicing:

- 1) The hearing aid must be serviced periodically to ensure long term usage.
- 2) The user must explore the possibilities of getting his/her hearing aid repaired/serviced in a place that is easily accessible.
- 3) It must be remembered that a hearing aid must have its troubles attended to, by a qualified personnel.
- 4) Nearness to a dealer is also important. If repair service is not immediately available, the user may be deprived of his instrument for longer periods of time.
- 5) Unnecessary repairs at exorbitant prices are to be avoided and the user should be careful against being 'High-pressured' into buying a new model of a hearing aid to substitute for an older model that happens to get out of order. So, the user must always contact a reliable person for repairs and servicing.

Purchase of components of the hearing aid:

- 1) At the time of sale, the hearing aid is given along with its accessories which include a receiver, an appropriate cord, an appropriate cell, a clip for a body worn hearing aid. These are placed in a case which gives adequate protection against dust and dirt.
- 2) The user would benefit, if he actually learns to connect the various accessories, prior to leaving the shop.
- 3) More important, he must make sure that he is getting the hearing aid, that was recommended for his use. The particulars regarding the model, recommended for his use, are normally inscribed on the hearing aid. Similarly, information on the receiver type can be seen on the receiver.

- 4) After connecting the accessories, the functioning of the hearing aid should be checked. Is the sound amplified and transmitted to the ear properly? Is the sound continuous or intermittent? Is there unnecessary noise, when the switches, volume control is moved around? Are there loose contacts or broken parts? All these points should be checked carefully.
- 5) Hearing aids in addition to varying in size and power differ in some other respects. For instance, some hearing aids are equipped with circuitry that will permit using the hearing aid with telephone, while cutting out the background noise, that would otherwise interfere with conversation.

Some hearing aids are meant for people who are unable to tolerate loud sounds even though they have hearing loss. This type of hearing aid would be recommended by the audiologist after confirming that the patient has a tolerance problem.

These and other factors are taken into consideration at the time of hearing aid trial and recommendations for the appropriate model are made. But the user should check all these points and must have a hearing aid trial prior to purchasing the same hearing aid.

- 6) In addition to these technical aspects, consideration for selection of a particular model may include recurring expenditure in replacing batteries, other accessories as the cord, receiver and switches.
- 7) While purchasing spares, the following points should be noted. You should always buy only the recommended spares.

a) Type of receiver - The type of receiver purchased has to be as recommended by an audiologist. Always matching receivers has to be purchased. Washer on the receiver should be intact, otherwise there would be leakage of sound energy.

b) Cord - Cords should be purchased according to the prescription by the audiologist. Cord length should be appropriate i.e., 50 cms. Make sure of the type of the cord whether it is 2 pin or 3 pin and whether it is a single V or Y cord. Cord should be checked carefully to detect any breaks along its length. Keep a spare cord, particularly if the dealer is not near.

c) Cell - Type and size of cell should be checked. All pen torch cells do not fit with all the hearing aids, find out which will be most appropriate for your hearing aid.

Different types of cells; pen torch cells, button cells are used with different hearing aids. Of these, the pen torch cells are easily available and they are less expensive. It has a voltage of 1.5 volts and is most commonly used with body worn hearing aids. The button cells are used with hearing aids worn at the ear level and are more expensive.

Periodical replacement of the cells should be done. For getting optimum usage, a regular user, must change hearing aid cells once in 8-10 days for body level hearing aids. For ear level hearing aids, where button cells are used, generally cells should be replaced after 100 hours of usage.

There are special cells which can be recharged and used again. These cells may be available with the dealer.

Process of recharging the cell is not economical in body level hearing aids as -

A cell in body level hearing aids, costs less and at the more two or three cells may be needed in a month for a regular user.

Purchase of rechargeable cells for the ear level hearing aid is recommended as it is economical.

d) **Volume control** - Whether it is numbered or not. Check if the switch is rotating smoothly or not.

e) **Tone control** - Whether it is present and functioning well or not. If it is internal, then adjustments should be done by the dealer before the user purchases a hearing aid.

f) Check for the presence of a separate on-off switch.

g) **Earmolds** :- If provided by the company, see if they fit properly. Some of the dealers provide eartips i.e., small plastic tubes instead of earmolds. But it is advisable, to get custom earmolds done as they fit properly.

h) **Telecoil** :- Whether it is present or not, especially for adult cases who are frequent telephone users. If present whether functioning well or not.

i) **Dust cover** :- It is provided with some hearing aid models to avoid dust collecting on the hearing aid switches.

j) Check for the hearing aid clip in body worn hearing aid to keep the hearing aid properly when worn on the body.

8) Serial number of a hearing aid is also important in identification of your hearing aid.

The information pertinent to hearing aid type, model and serial number helps -

- 1) In the identification of your hearing aid in the event of loss/theft.
- 2) In ensuring that you receive the same hearing aid after repair.
- 3) In giving complete information regarding your hearing aid to the audiologist.

Cost :

It is an important factor in purchase of hearing aid. Before purchase, you should ask the audiologist regarding the cost of the prescribed hearing aid.

Sometimes, the dealers may try to mislead the purchaser. Some dealers may charge for the hearing aid depending on patient's/parent's income. So a purchaser should be aware of such practices. He should check the cost factor carefully before the purchase.

Also, the purchaser must ask for a receipt and the guarantee card which must be filled in. This helps in getting the repairs done free of cost during the guarantee period.

The buyer must get the guarantee card filled. In some cases, guarantee cards are not given. Even if they are given the details are not filled out, or the card is given but it is taken back on a subsequent visit. The user should be aware of such practices.

Thus, before purchase of a hearing aid, three major items of expense should be noted as - the initial cost, repairs and replacement, cell expenses. Low cost of one of these items does not necessarily means low cost of others.

It is also recommended that the hearing aid be tried on the patient and its utility established, before purchase of a hearing aid. After purchase, every user should visit the audiologist to ensure that he has received the right hearing aid.

The purchaser must remember that a hearing aid should be accompanied by the following information as -

- 1) Illustration of the hearing aid showing controls, adjustments and cell compartments.
- 2) Printed material on operation of all controls designed for user adjustment.
- 3) Description of possible accompanying accessories such as telecoil for specialized provisions for listening over telephone.
- 4) Instructions on how to use, maintain and care for, as well as replace or recharge the cells.
- 5) How to and where to get the hearing aid repaired.
- 6) Conditions to be avoided in preventing damage to hearing aids, such as dropping or exposing to excessive heat or humidity.
- 7) Selected electroacoustical data obtained in accordance with the respective standard (this information may be included on separate labeling that accompanies the hearing aid).

If the above points are kept in mind, the chances of an individual with hearing loss, purchasing an aid that suits him best and to derive maximum benefit from it are maximised.